

## TOXO IgG/IgM Rapid Test Kit Instructions For Use

### PRODUCT NAME

ENO TOXO IgG/IgM Rapid Test Kit

### PACKAGE SPECIFICATION

40 tests/kit

### INTENDED USE

ENO TOXO IgG/IgM Rapid Test is a lateral flow chromatographic immunoassay for the simultaneous detection and differentiation of anti-Toxoplasma gondii (T. Gondii) IgM and IgG in human serum or plasma. It is intended to be used by professionals as a screening test and provides a preliminary test result to aid in the diagnosis of infection with T. gondii.

### SUMMARY AND PRINCIPLES OF THE PROCEDURE

T. gondii is an obligate intracellular protozoan parasite with a worldwide distribution. Serological data indicates that approximately 30% of the population of most industrialized nations is chronically infected with the organism. A variety of serological tests for antibodies to T. gondii have been used as an aid in diagnosis of acute infection and to assess previous exposure to the organism. These tests are the SabinFeldman dye test, direct agglutination, indirect hemagglutination, latex agglutination, indirect immunofluorescence and ELISA. Recently, lateral flow chromatographic immunoassay, such as the ENO TOXO IgG/IgM Rapid Test, was introduced into the clinic for the serodiagnosis of T. gondii infection.

ENO TOXO IgG/IgM Rapid Test is a lateral flow chromatographic immunoassay. In this test, mouse anti-human IgM and IgG are coated in the test line regions of the test. During testing, the serum, plasma or whole blood specimens react with TOXO antigen-coated gold particles in the label pad. The mixture then migrates forward on the membrane by capillary action and reacts with the mouse antihuman IgM and IgG on the membrane in the test line regions respectively. The presence of a colored line in the test line (G) region indicates a positive result for TOXO antibody IgG, the presence of a colored line in the test line (M) region indicates a positive result for TOXO antibody IgM, while any absence indicate a negative result for that infection. To serve as a procedural control, a coloured line will always appear in the control reaction zone (C) indicating that proper volume of specimen has been added and membrane wicking has occurred.

### MATERIALS PROVIDED

Each kit contains:

1. test cassettes: 40 pieces test cassettes individually pouched.
2. Wash Buffer Solution: 3.0 ml in dropper bottle.
3. Package insert: 1 piece attached.

### MATERIALS REQUIRED BUT NOT PROVIDED

- Timer or stopwatch.
- Specimen collection containers
- Disposable gloves and/or protective clothing
- Centrifuge (for plasma only)
- Micro-pipette

### WARNINGS

1. Read the package insert completely before using the product. The instructions must be followed carefully as not doing so may result in inaccurate results.
2. The kits for diagnostic use only.
3. Perform test at room temperature.

### PRECAUTIONS

1. ENO TOXO IgG/IgM Rapid Test Kit is for professional use only.
2. The package insert instructions must be followed to ensure optimum test performance.
3. The kit is intended for *in vitro* diagnostic use.
4. As with all screening assays, any results should be considered presumptive until confirmatory assays have been performed according to local practice or WHO guidelines.

### Safety Precautions

1. Standard precautions for handling infectious agents should be observed when using this kit.
2. Wear protective clothing such as lab coat, safety glasses and disposable gloves when handling specimens and assay reagents.
3. Wash hands thoroughly after use.
4. In case of contact with eyes, rinse immediately with plenty of water and seek medical advice.

### Bio safety Precautions

Appropriate bio safety practices should be used when handling specimens and reagents. These precautions include, but are not limited to the following:

1. Do not smoke, eat, drink, apply cosmetics or handle contact lenses in areas in which specimens are handled.
2. Dispose of all specimens, used devices and tubes as though they are capable of transmitting infection. The preferred methods of disposal are by autoclave at 121°C for a minimum of 60 minutes or by incineration. Disposable materials may be incinerated. Liquid waste may be mixed with appropriate chemical disinfectants. A solution of 10% bleach is recommended. Allow 60 minutes for effective decontamination. NOTE: Do not autoclave solutions containing bleach.
3. When disposing of solution, avoid contact with acid to prevent liberation of a toxic gas.
4. All spills should be wiped thoroughly using a suitable disinfectant such as a sodium hypochlorite solution.
5. Use a separate dropper and device for each specimen tested.

### Handling Precautions

1. Do not use if the kit safety seal is absent, damaged or broken.
2. Do not use any device if the pouches have been perforated.
3. Each device is for single use only.
4. Do not mix wash buffer solution/test cassettes from different kit lots.
5. Do not use the kit past the expiration date (this date is printed on the kit box).
6. Adequate lighting is required to read the test results.
7. The result should be read immediately after the end of the 10 minutes incubation time following the addition of specimen and wash buffer solution. Do not read results beyond 15 minutes.

### STORAGE INSTRUCTIONS

1. The kit should be stored between 2-30°C and the shelf life is 24 months.
2. The kit components are stable until the expiration date printed on the outer label, when stored as directed. The kit expiry date is determined by whichever of the components has the shortest expiry date. The kit expiry date is not impacted once the wash buffer solution has been opened. Do not use kit components beyond overall kit expiry date.
3. If stored refrigerated, ensure that the pouched device is brought to room temperature before opening.
4. Do not freeze the kit.

### SAMPLE COLLECTION AND PREPARATION

1. Applicable samples: Whole Blood/Serum/Plasma.

- Separate serum or plasma from whole blood as soon as possible to avoid hemolysis. Use only clear nonhemolysis specimens.
- Testing should be performed immediately after the specimens have been collected as soon as possible. Do not leave the specimens at room temperature for prolonged periods.
- Serum and plasma specimens may be stored at 2-8 °C for up to 7 days, for long term storage, serum/plasma specimens should be kept below -20°C. Whole blood collected by venipuncture should be stored at 2-8°C if the test is to be run within 2 days of collection.
- Do not freeze whole blood specimens.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly.
- If specimens are to be shipped, they should be packed in compliance with local regulations covering the transportation of etiological agents.
- EDTA K2, Heparin sodium, Citrate sodium and Potassium Oxalate can be used as the anticoagulant for collecting the specimen.

#### QUALITY CONTROL

An internal procedural control is included in the test, a colored line appearing in the control line region (C) is an internal valid procedural control, it confirming adequate membrane wicking. Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

#### TEST PROCEDURE

Allow the test cassette, specimen, buffer solution to equilibrate to room temperature (15-30°C) prior to testing.

- Remove the test cassette from the sealed pouch and use it within one hour. Place the test cassette on a clean and level surface.
- For Serum or Plasma Specimens

To use a dropper: Hold the dropper vertically, draw the specimen and transfer the specimen to the sample well of the test cassette (one drop/approximately 10ul), then squeeze the wash buffer solution bottle, add three drops wash buffer solution inside (approximately 90ul) to the sample well and start the timer. Avoid trapping air bubbles in the sample well.


To use a micro-pipette: Pipette and dispense 10ul of specimen to the sample well of the test cassette, then squeeze the wash buffer solution bottle, add three drops wash buffer solution inside (approximately 90ul) to the sample well and start the timer.

#### For Whole Blood Specimens

To use a dropper: Hold the dropper vertically, draw the specimen and transfer the specimen to the sample well of the test cassette (two drops/approximately 20ul), then squeeze the wash buffer solution bottle, add three drops wash buffer solution inside (approximately 90ul) to the sample well and start the timer. Avoid trapping air bubbles in the sample well.

To use a micro-pipette: Pipette and dispense 20ul of specimen to the sample well of the test cassette, then squeeze the wash buffer solution bottle, add three drops wash buffer solution inside (approximately 90ul) to the sample well and start the timer.

- Wait for the colored line(s) to appear. The test result should be read at 10 minutes. Do not interpret the result after 15 minutes.

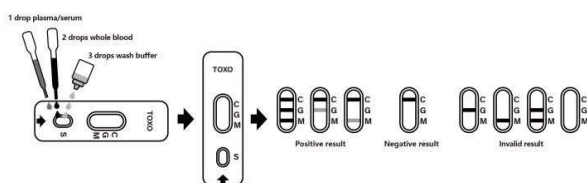

#### INTERPRETATION OF RESULTS

**IgG and IgM POSITIVE:** Three lines appear. One colored line should be in the control line region(C), and two colored lines should appear in IgG test line region and IgM test line

**IgG POSITIVE:** Two lines appear. One colored line should be in the control line region(C), and a colored line appears in IgG test line region. The result is positive for TOXO specific-IgG and is probably indicative of secondary TOXO infection.

**IgM POSITIVE:** Two lines appear. One colored line should be in the control line region (C), and a colored line appears in IgM test line region. The result is positive for TOXO specific-IgM antibodies and is indicative of primary TOXO infection.

**NOTE:** The intensity of the color in the IgG and/or IgM test line region(s) will vary depending on the concentration of TOXO antibodies in the specimen. Therefore, any shade of color in the IgG and/or IgM test line region(s) should be considered positive

**NEGATIVE:** One colored line should be in the control line region (C). No line appears in IgG and IgM test line region(s)

**INVALID:** Control line fails to appear. Insufficient buffer volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the procedure with a new test cassette. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

#### LIMITATIONS

- The kit is for in vitro diagnostic use only. The test should be used for the detection of TOXO IgG/IgM antibodies in serum, plasma or whole blood specimens only.
- A negative test result cannot exclude a recent infection. A positive result may not indicate previous TOXO infection. Consider other information including clinical history and local disease prevalence, in assessing the need for a second but different serology test to confirm an immune response.
- A negative or non-reactive result can occur if the quantity of the anti-TOXO antibodies present in the specimen is below the detection limits of the assay or the antibodies that are detected are not present during the stage of disease in which a sample is collected.
- Results from this test should not be used to diagnose or to exclude acute TOXO infection or to inform infection status.

#### Cross Reaction

ENO TOXO IgG/IgM Rapid Test Kit was tested with specimens from patients diagnosed with HAV, HBV, HCV, HEV, HIV, RF, Syphilis, HAMA, Mononucleosis positive specimens. The results showed no cross reactivity

#### PERFORMANCE CHARACTERISTICS

The color intensities of the lines do not have to match. The result is positive for IgG & IgM antibodies and is indicative of secondary TOXO infection.

Total Results	71	681	752
---------------	----	-----	-----

#### TOXO IgG Study Summary Results:

Clinical sensitivity =95.77% (95%CI\*88.14%~99.12%)

Clinical specificity=99.12% (95%CI\*98.09%~99.68%)

Accuracy=98.80% (95%CI\*97.74%~99.45%)

#### Interference Substances

The following potential interfering substances have been tested using The kit and no interference was observed:

Substance	Tested Concentration
Antinuclear antibody (ANA)	100 IU/mL
Anti-mitochondrial antibody(AMA)	80 U/mL
Human albumin	110 mg/mL
Bilirubin	1 mg/mL
Hemoglobin	10 mg/mL
Cholesterol	0.2mg/ml
Triglycerides	15 mg/mL

**ENOLAB MEDIKAL**  
SANAYI VE TICARET LIMITED SERKETI

**www.eno-lab.net**  
**Email: info@eno-lab.net**  
**cumhuriyet mah serife baci cad. B blok**  
**No : 3Ag Corlu/TEKIRDAG**